

FIG. 1 (A)

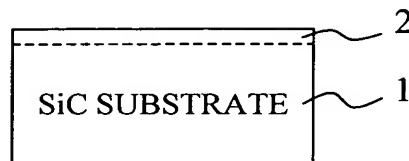


FIG. 1 (B)

HF AQUEOUS SOLUTION TREATMENT

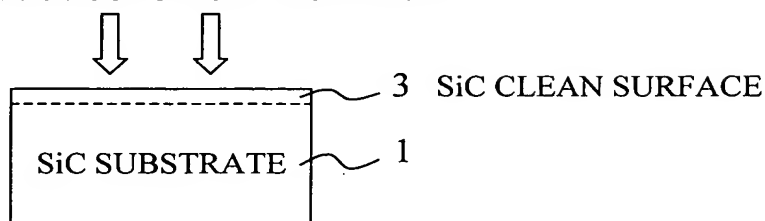


FIG. 1 (C)

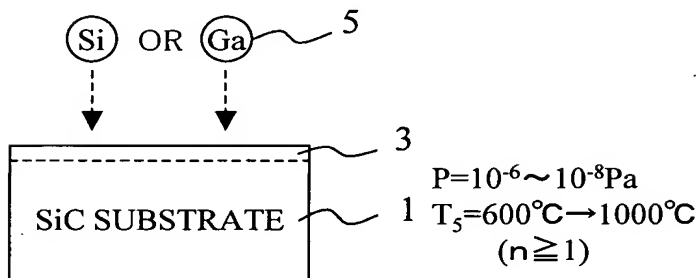


FIG. 1 (D)

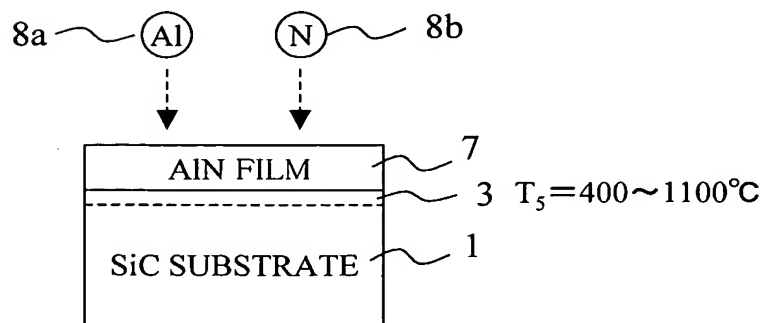


FIG. 2 (A)

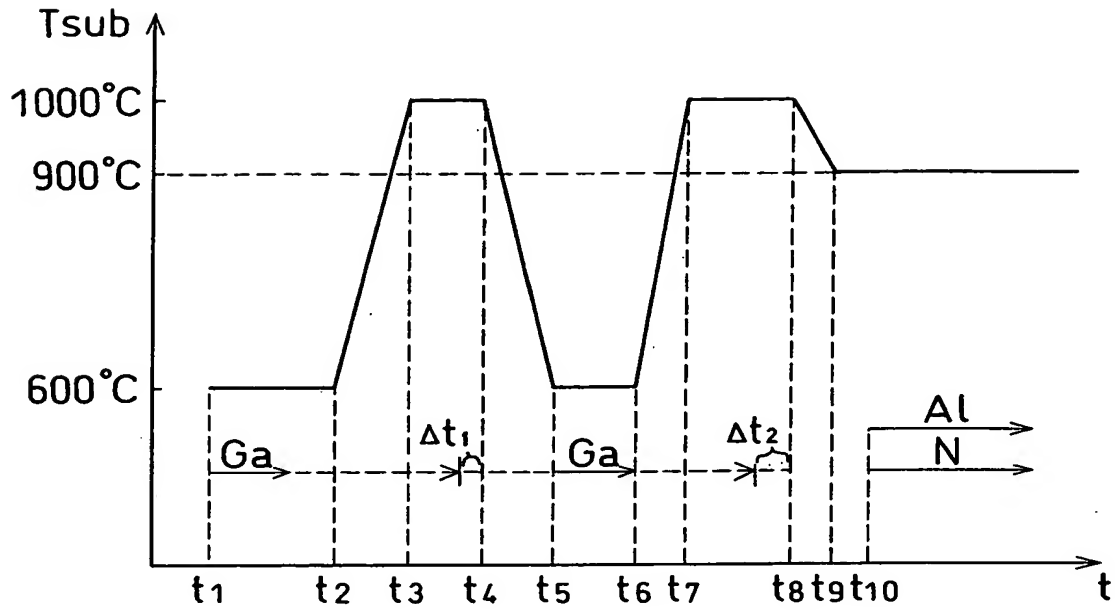


FIG. 2 (B)

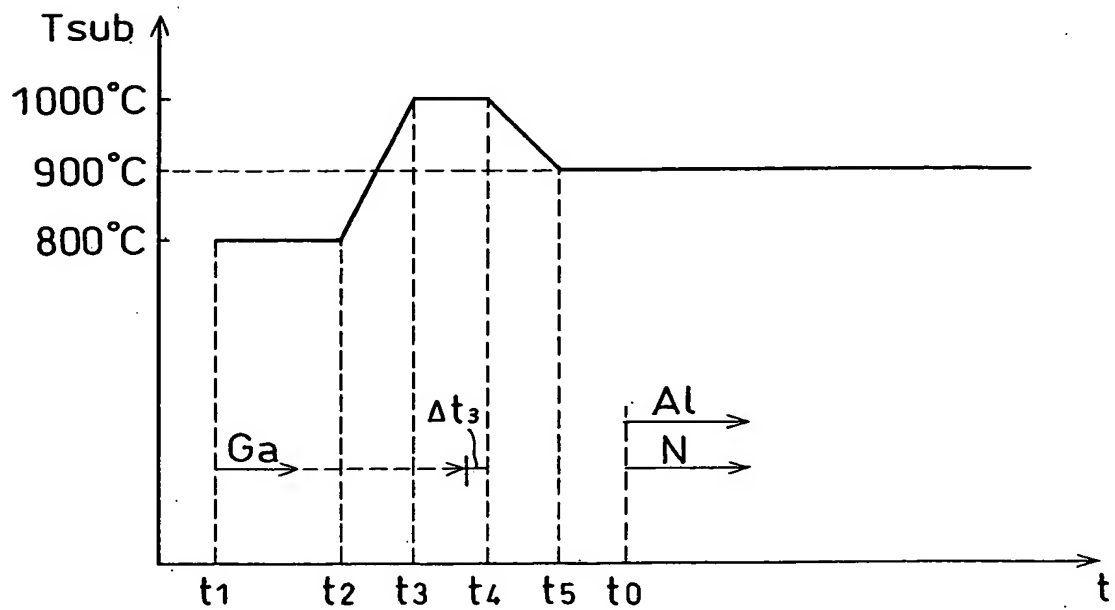


FIG. 3 (A)

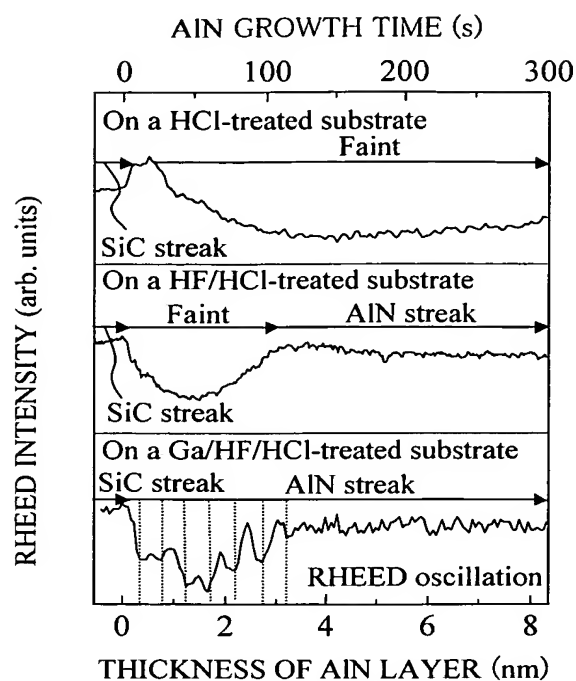


FIG. 3 (B)

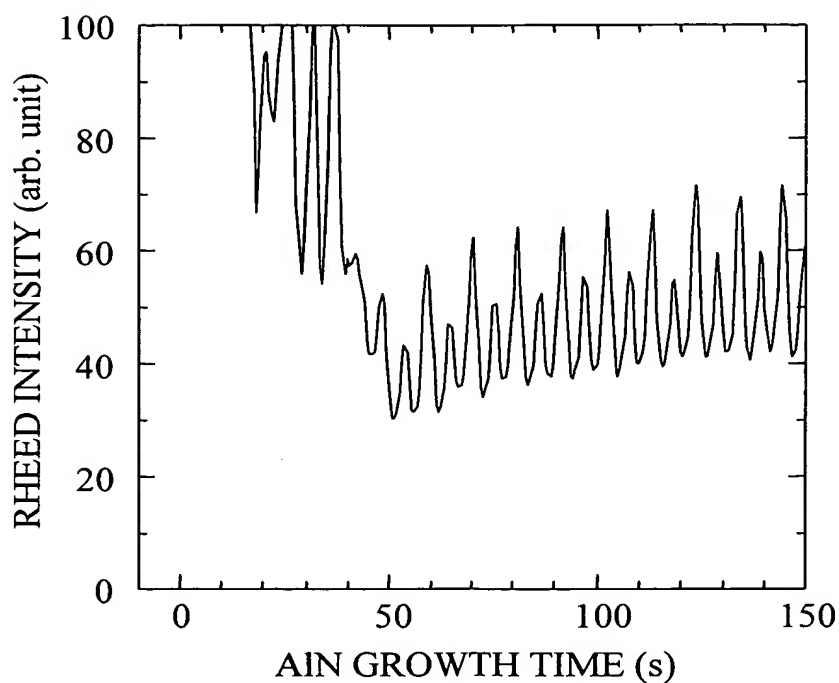


FIG. 4

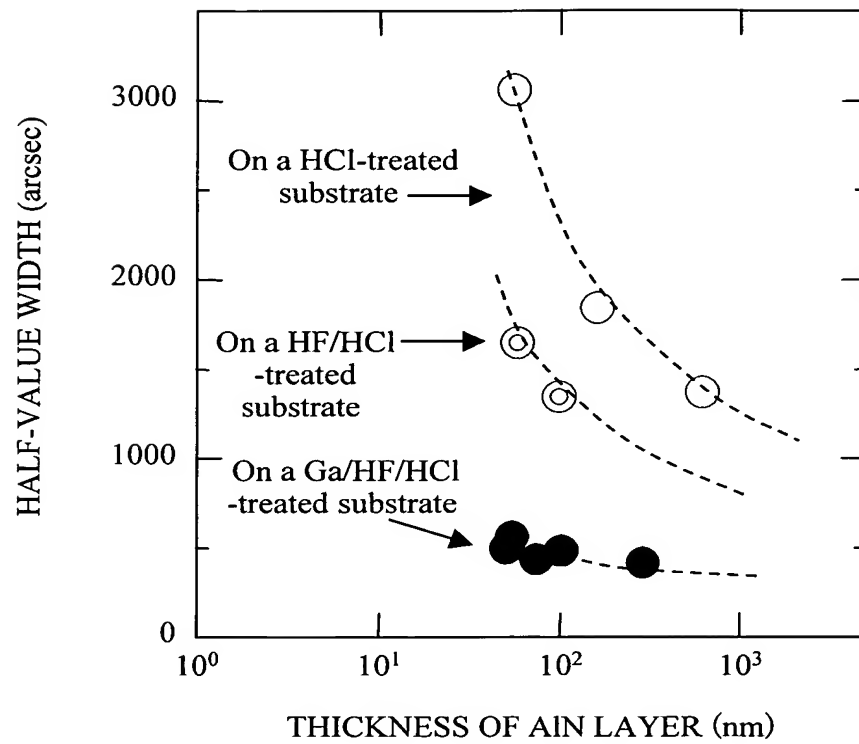


FIG. 5 (A)

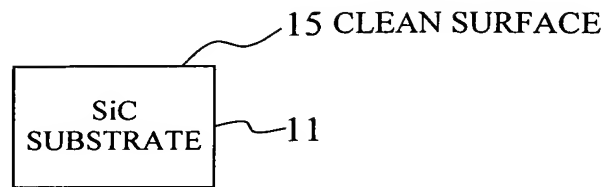


FIG. 5 (B)

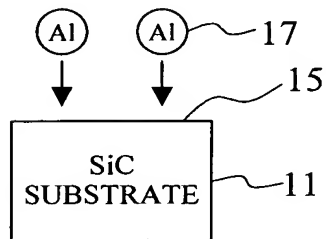


FIG. 5 (C)

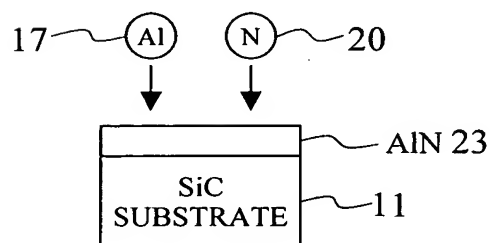


FIG. 6

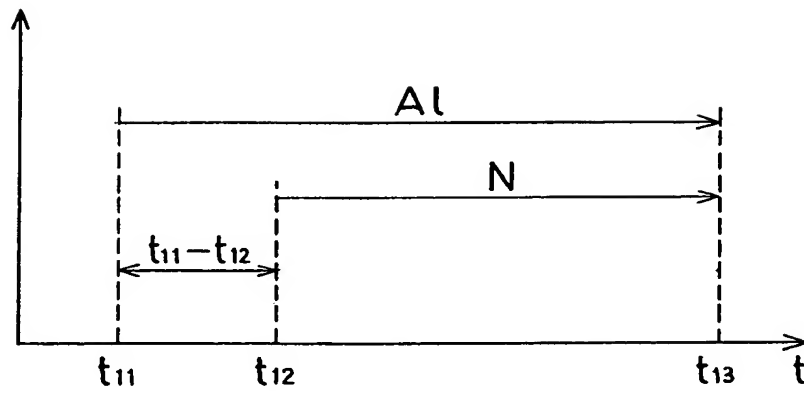


FIG. 7 (A)

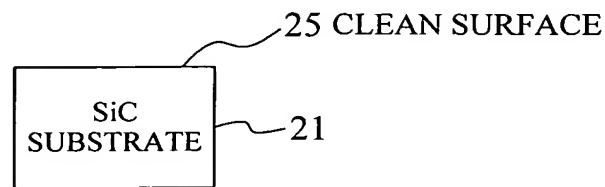


FIG. 7 (B)

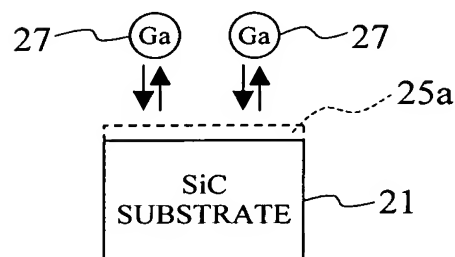


FIG. 7 (C)

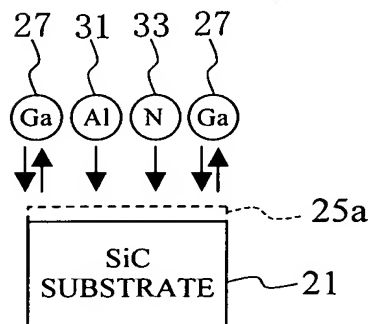


FIG. 7 (D)


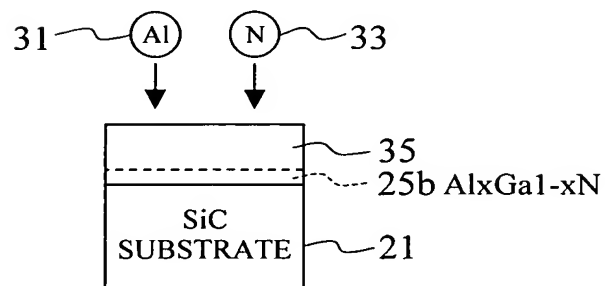


FIG. 8



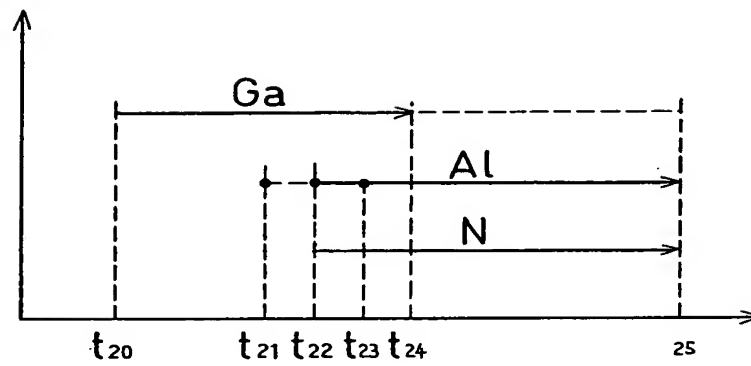

10/549683

FIG. 9 (A)

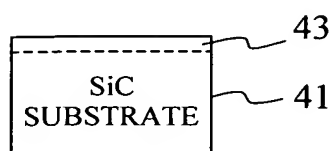


FIG. 9 (B)

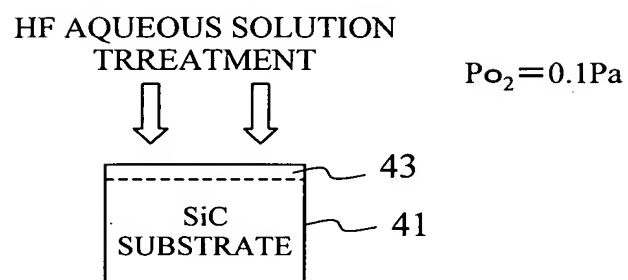


FIG. 9 (C)

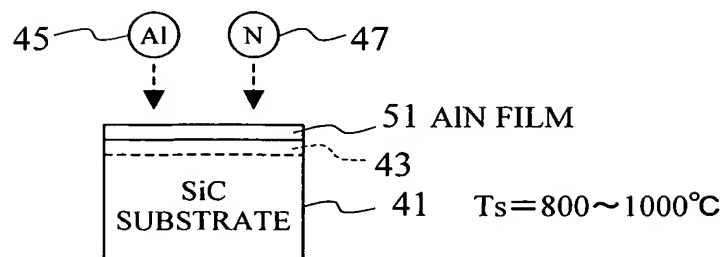


FIG. 10 (A)

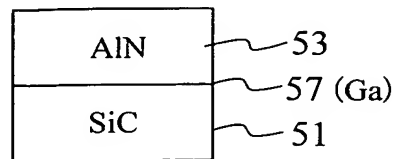


FIG. 10 (B)

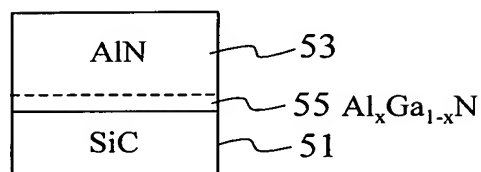


FIG. 10 (C)



FIG. 10 (D)

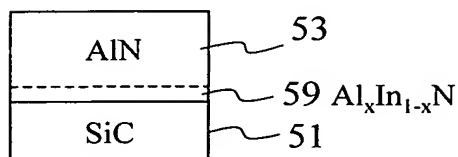


FIG. 11 (A)

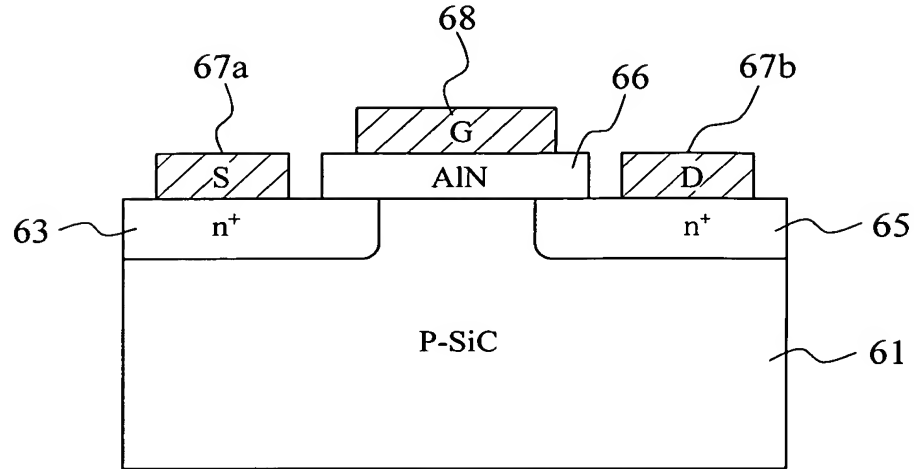


FIG. 11 (B)

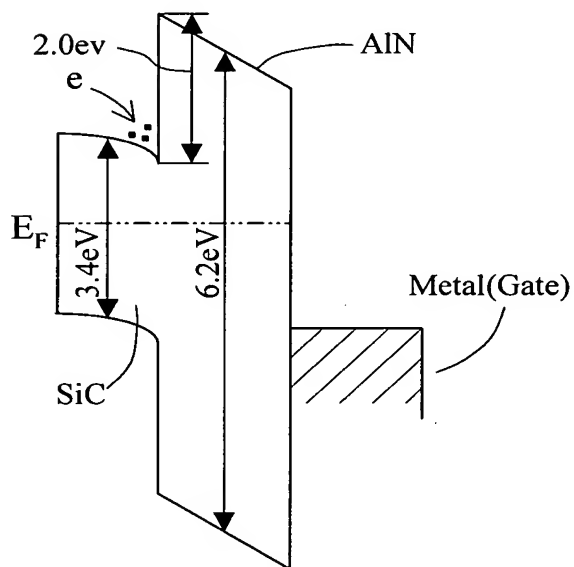


FIG. 12

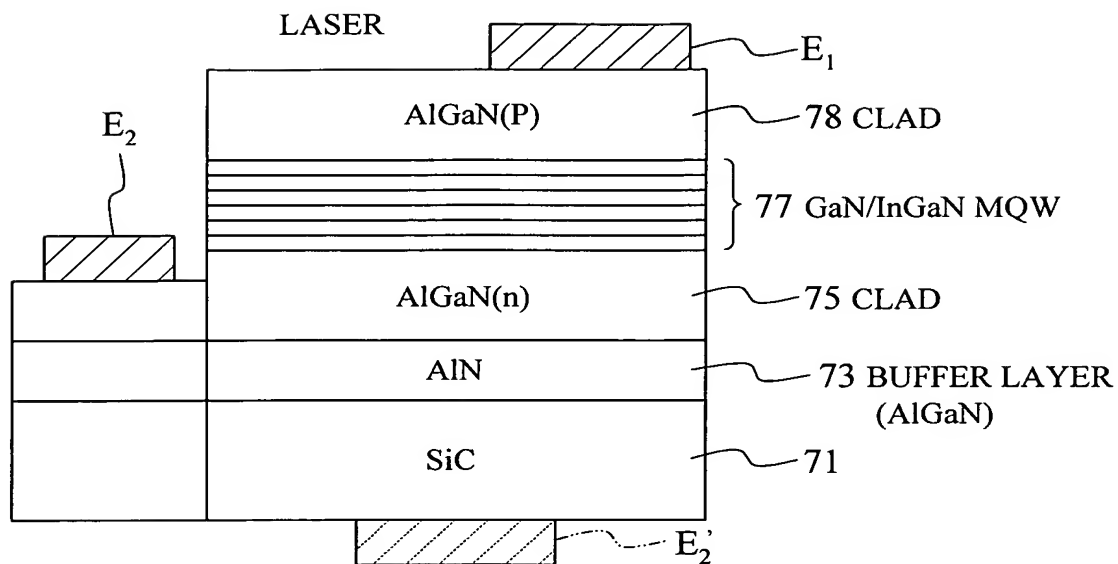


FIG. 13

